

Backup Air Dehydrator For Dental Operating Room

Features

- Complete Instrumentation Package to Monitor Operation
- Low Purge Loss
- Purge Air Consumption Does Not Increase with Increasing Inlet Pressure
- No Electrical Power Needed

General Description

The Model 7005 series air dehydrator has been selected for the LPD 17 San Antonio class. It is designed to provide up to 7 scfm of clean, dry air for use in shipboard dental operating rooms. The unit is fully automatic and operates with very little maintenance.

The Model 7005 includes a coalescing filter (removes 100% of 0.03 micron or larger diameter solids and liquid particles), a membrane dehydrator, and upstream and downstream isolation valves.

Specifications

Built in accordance with LPD 17 Specification 6259K. Welded in accordance with S9074-AR-GIB-010/278. Fully qualified to MIL-S-901C, High Impact Shock (Grade B), and MIL-STD-167-1, Vibration (Environmental) Shipboard.

Outlet Capacity: 0 - 7 scfm.

Inlet Air Conditions (defined by specification): 80-125 psig, 50° F to 122° F, maximum dew point of 60° F at 80 psig.

Outlet Air Conditions: Dew point -40° F or lower at pressure. Pressure not more than 10 psig below inlet.

Electrical Requirements: None.


Dimensions: 16" W x 48" H x 12" D

Weight: 77 pounds

APL: To be determined.

Technical Manual: Mark I: TM7005-MI-00

QA System: ISO-9001 - 1994

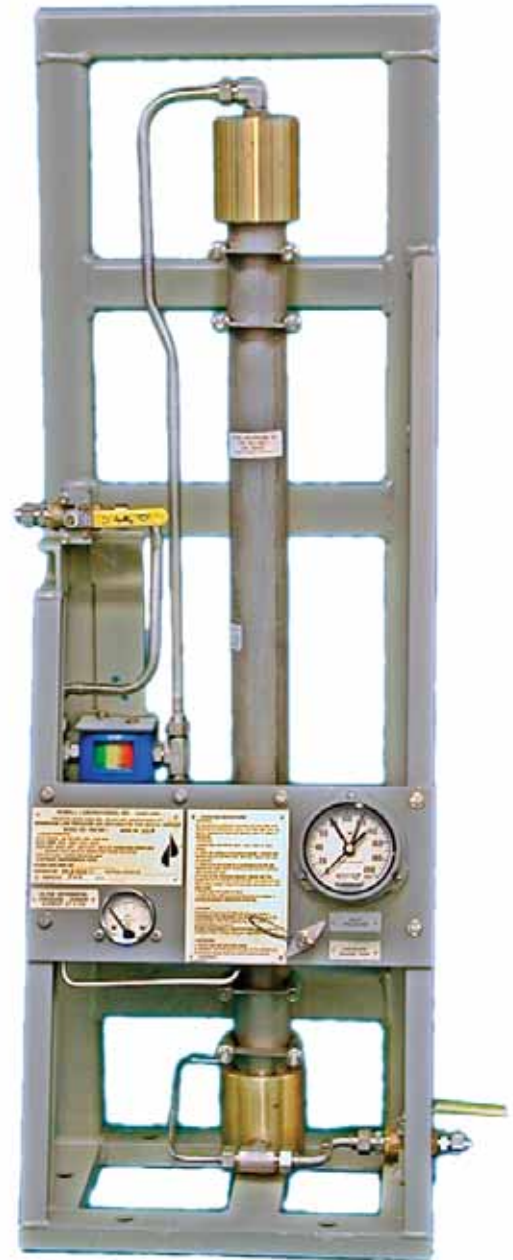

Howell Laboratories, Inc.

188 Harrison Rd.
Bridgton, Maine 04009
(207) 647-3327

(888) 744-8359

FAX (207) 647-8273

e-mail: contracts@howelllabs.com
An Employee-Owned Company

web: www.howelllabs.com
Certified to ISO 9001:2000